

Barrier Technique

The first choice in the protection of dental equipment should be the use of disposable barrier products. The repeated use of disinfectants on equipment surfaces without the constant removal of the solution residue will eventually cause some damage to equipment surfaces.

Chemical Disinfection

The manufacturer of the disinfectant to be used should be contacted for them to state that the disinfectant will not damage equipment surfaces including upholstery.

Unacceptable Disinfectants

The following chemicals may damage equipment and upholstery:

- * Alcohol based solutions
- * Bleach
- * Phenol/Alcohol combinations
- * Foam spray products

Use with Caution

* Water based phenolic disinfectants following exactly the instructions for use.

The Belmont Warranty does not cover damage to equipment and upholstery caused by disinfectant solutions.

WARRANTY -

Belmont Equipment is warranted by the manufacturer to be free from defective material and workmanship under normal use and service, for a period of two (2) years' from date of shipment to the Buyer, except that any part or parts that are replaced under this Warranty within ninety (90) days of the completion of the two year period shall be warranted to be free from defective material and workmanship for a period of ninety (90) days from date of shipment of said parts to Buyer. Belmont will repair or replace any defective part under this Warranty, provided the part is returned to our factory with prepaid postage, delivery or freight charges. In the event Warranty service must be performed to correct any defect, only Belmont and/or one of its authorized dealers shall provide same upon mutually agreeable arrangements made in advance.

Except as otherwise provided herein, there is NO WARRANTY, representation or condition of ANY KIND, express or implied (including NO WARRANTY OF MERCHANTABILITY OR FITNESS) and none shall be implied by law. THE EXPRESS WARRANTY AND THE REMEDIES CONTAINED HEREIN (1) ARE MADE SOLELY TO THE FIRST PURCHASER FOR BENEFICIAL USE (THE BUYER), (2) ARE THE SOLE WARRANTIES AND REMEDIES, (3) ARE IN LIEU OF ALL OTHER WARRANTIES, GUARANTEES, AGREEMENTS OR OTHER LIABILITIES, WHETHER EXPRESS OR IMPLIED, AND ALL OTHER REMEDIES FOR BREACH OF WARRANTY OR ANY OTHER LIABILITY OF BELMONT. IN NO EVENT SHALL BELMONT BE LIABLE FOR CONSEQUENTIAL OR INCIDENTAL DAMAGES.

No person, agent, distributor or dealer is authorized to change, modify or extend the terms of the Warranty in any manner, whatsoever.

This warranty is void when failure or defect is caused by conditions beyond the manufacturer's control, such as damage resulting from mishandling, neglect, misuse, improper maintenance, accident or alteration or repair by anyone other than Belmont or an authorized Belmont dealer.

Labor required to repair, replace or retrofit is not included during the warranty period by the manufacturer.

CONTENTS

INSTALLATION AND ASSEMBLY Unit Installation	2
Unit Installation Handpiece Tubing	4
CONTROL FUNCTIONS	
Automatic Handpiece Control	5
FINAL ADJUSTMENTS	6
SERVICE AND MAINTENANCE	
Syringe	7

SCHEMATIC

Doctor's Handpiece Control System, 3 HP Automatic Single Water Bottle Schematic

PARTS & SERVICE DRAWINGS

Single Water Bottle System

INSTALLATION AND ASSEMBLY

UNIT INSTALLATION

- Fasten the unit swivel plate to the underside of the sliding work surface using the four 10-24 machine screws provided. See Figure 1.
- Route the unit umbilical through the cabinet to the floor utilities and make the proper connections.

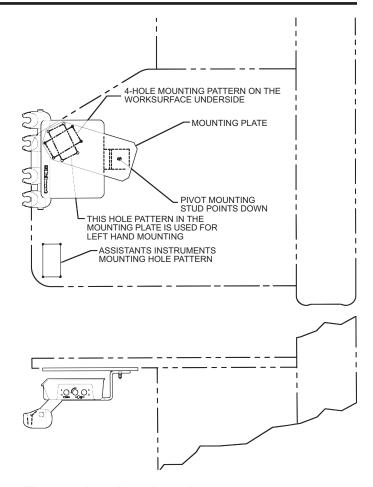
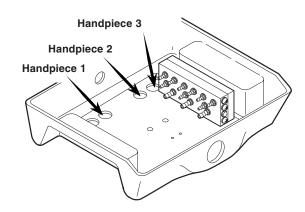


Figure 1. Installing the unit.

REPLACING HANDPIECE TUBING

INSTALL HANDPIECE TUBING See Figure 2

- 1. Remove the control from the swivel bracket.
- 2. Remove the lid from the handpiece control.
- 3. Open the handpiece tubing packages, measure the length needed and snip.
- 3. Feed the tubing up through the hole in the handpiece control and connect the tubing to the appropriate barb connections on the tri-block.
- 4. Repeat Step 3 for the remaining tubings.
- 5. After the tubings are connected and there are no leaks, replace the lid.



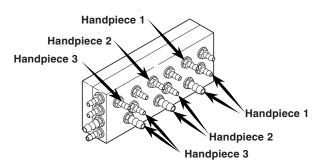


Figure 2. Installing the handpiece tubing.

HANDPIECE CONTROL FUNCTIONS

All controls are located on the side panels. With the exception of the water coolant on/off which is located on the foot control. Figure 3 shows the location and identifies the function of these controls.

WATER COOLANT ON/OFF

Located on the foot control this activates handpiece water coolant system. Flip the toggle to activate the system.

WATER COOLANT FLOW CONTROL

Allows adjustment to be made to the handpieces. Turn the knob counter clockwise to increase the flow, clockwise to decrease the flow.

MASTER ON/OFF

Turns on air and water for the complete system. Flip the toggle up to activate the system. Always turn the toggle OFF whenever unit is not in use.

DRIVE AIR PRESSURE GAUGE

Indicates drive air pressure to the handpiece.

DRIVE AIR PRESSURE CONTROL

Allows handpiece to be adjusted to its manufacturer's recommended operating pressure. Turn the adjusting screw counter clockwise to increase the pressure, clockwise to decrease the pressure.


Figure 4 shows the automatic handpiece holder and syringe holder assembly.


AUTOMATIC HANDPIECE HOLDER

Signals the automatic control system to supply drive air and air/watercoolants to the handpiece as it is lifted from its holder. When the handpiece is placed back in the holder, a signal to the automatic control system stops the drive air and air/water coolant supply.

FOOT CONTROL

Regulates drive air and water to the active handpiece. To operate, apply pressure to the foot control for drive air.

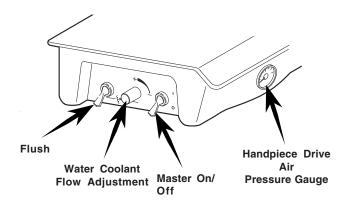



ment
(3 places)
Figure 3. Handpiece control functions.

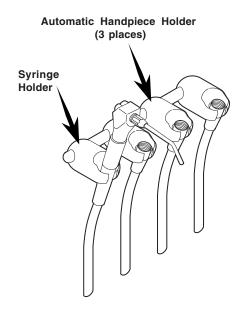


Figure 4. Automatic handpiece holder assenbly.

FINAL ADJUSTMENTS

FINAL ADJUSTMENTS

Adjust the air and water regulated pressure.

Adjust the handpiece pressure.

Check for any leaks.

SYRINGE

TIP STERILIZATION

- 1. To remove Syringe Tip, firmly grasp tip and pull away from Syringe head.
- 2. Replace the tip by inserting a new one into the tip socket, and firmly pushing into place until you feel it softly "pop" into place. To ensure it has been fully inserted, the uppermost small groove on the tip shank must be just visible over the end of the socket. See Figure 5.

NOTE

Be sure to rinse all cleaning agents from the tip prior to sterilization. You may sterilize Syringe Tips by any of the following methods; Chemical Vapor, Ethylene Oxide or Steam Autoclave. Temperatures should never exceed 280 degrees Farenheit, (138 degrees Celsius).

INSTALLATION

- 1. Turn off Air and Water supplies.
- 2. Unscrew Syringe handle and determine which fitting leads to the air button.
- 3. Slide the Syringe handle down over the syringe tubing. Select the air side of the syringe tubing and connect to the air fitting on the syringe.

4. Repeat with the water tubing to the water fitting. Ensure that the unit end of the Syringe tubing is properly connected to the air and water supply fittings on the dental unit. Recommended operating pressures: Air 80 psi, Water 40 psi.

This groove must be

just visible above tip of conical socket.

TROUBLE SHOOTING

Problem: Water leakage around buttons.
Solution: Replace the button assembly

C-1701 (See figure 5). Turn water and air supply off. Depress air and water buttons on Syringe to relieve residual pressure. Hold both buttons down and use a paperclip to push cross pin out of syringe head. Gently remove button from head, being careful not to lose conical spring beneath. To install new button, ensure that conical spring is seated with the small end pointing up. Gently push into place and hold both buttons down firmly while re-inserting cross-pin.

Problem: Solution:

Water spray when air button is pressed. Ensure tip is properly and fully inserted. If so, replace O-ring #R-C16004 (See Figure 5). Twist conical tip socket assembly (R-C21600-3) off of syringe head to access this O-ring. When re-installing tip socket assembly, hand tighten only. If tip cannot be fully inserted, then socket is too tight.



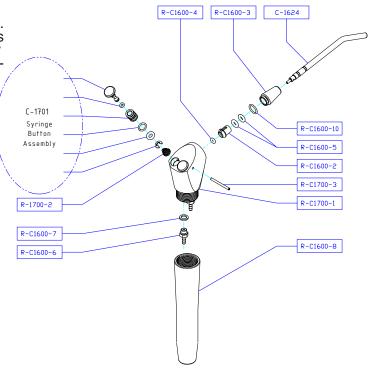


Figure 5. Syringe.

REF. NO.	DESCRIPTION PART NO.	QTY.
1	AUTOMATIC HANDPIECE CONTROL, TRI-BLOCK 1100-170	1
2	CONTROL HOUSING	1
3	SCREW, 4-40 x 1/4" ALLEN BUTTON HEAD0012-410	2
4	GAUGE BRACKET CONTROL0023-529	1
5	FITTING, 1/4" POLY x 1/8" FPT0016-006	1
6	7/8" DIA. GAUGE0020-030	1
7	AUTOMATIC HP HOLDER FGTA11A0	3
8	HOLDER BAR EXTENSION0024-162	1
9	HOLDER BAR0024-075	1
10	SYRINGE HOLDERFGTA12A0	1
11	SCREW, 1/4-20 x 1/4" S.S. SET SCREW0012-250	1
12	TOGGLE VALVE, ON/OFF, 3-WAY, OUTPORT 1100-401-X	1
13	DECORATIVE TRIM NUT, SMOOTH, SILVER0013-016	3
14	NEEDLE VALVE ASSEMBLY 1100-100-X	1
15	TOGGLE VALVE, ON/OFF, 3-WAY, OUTPORT 1100-400-X	1
16	FLOW RESTRICTOR1100-130	1
17	SCREW, 10-32 x 3/8" S.S. BUTTON HEAD0012-136	4
18	FITTING, 10-32, 4-WAY CROSS, FEMALE0016-060	2
19	SCREW, 10-320012-021	1
20	NUT, LOCKING0013-024	1
21	WASHER 1" 0011-016	1
22	UNIT BRACKET 0023-602	1
23	BUSHING0006-015	1
24	RETAINER	1
25	WATER PILOT VALVE, 2 WAY, W/O EXHAUST, 1100-145	1
26	WASHER, 2" 0011-015	1
27	NUT, 10-32, KEP, ZINC0013-008	2
28	SHUTTLE VALVE1100-140	1
29	SWIVEL BRACKET 0023-610	1

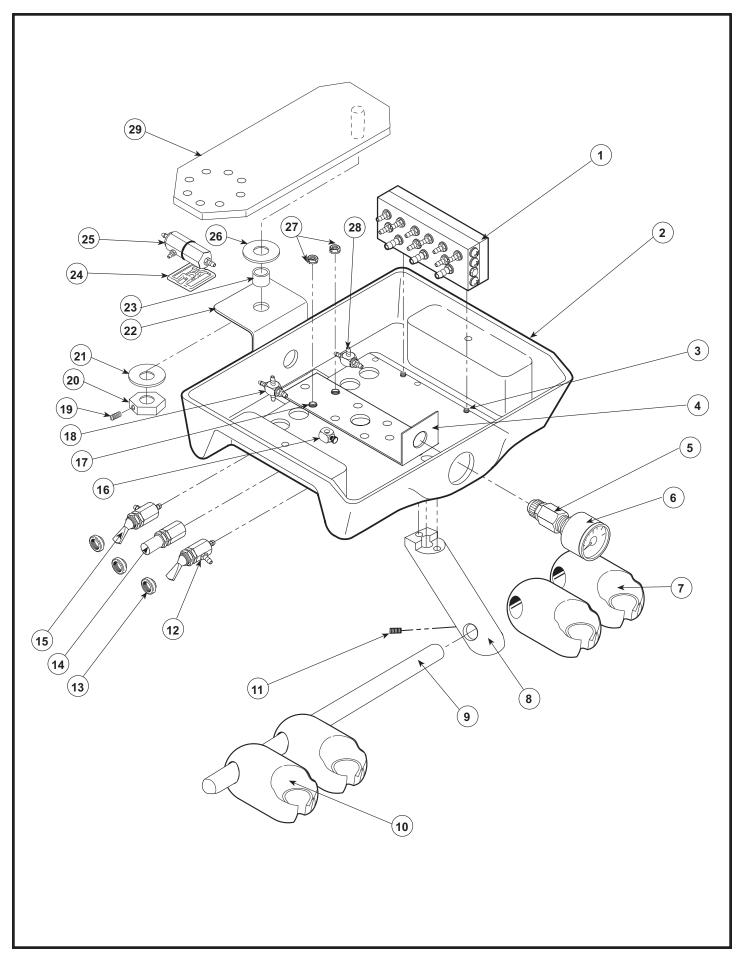

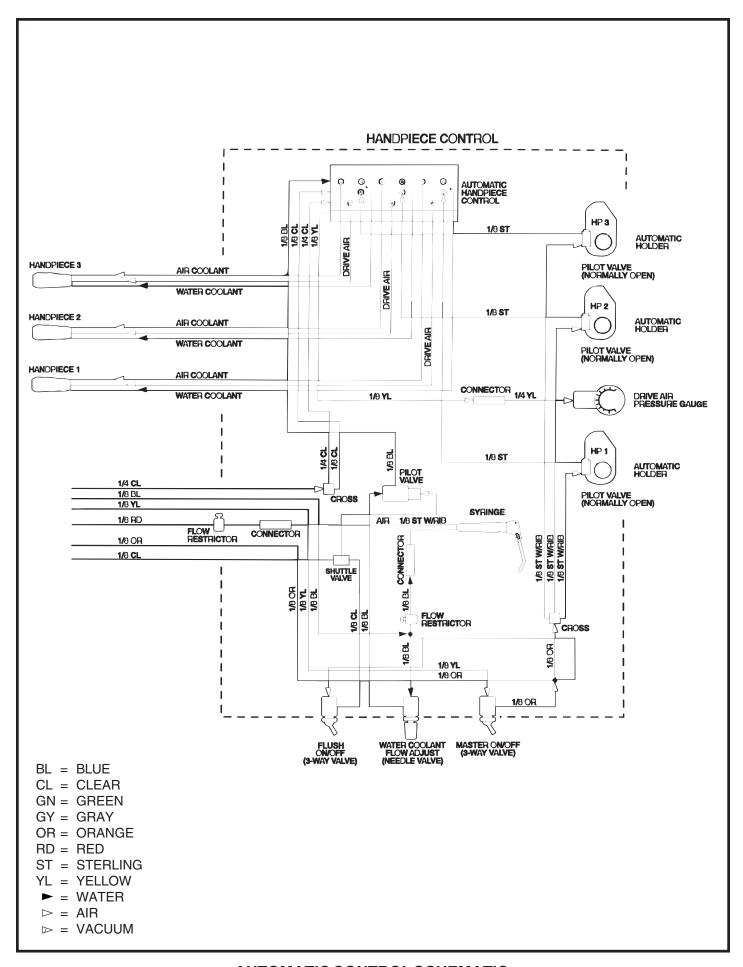

= VACUUM

► = WATER

