Belmont

X-CALIBUR UNIT

FLOOR TEMPLATE
for BEL20 CHAIR

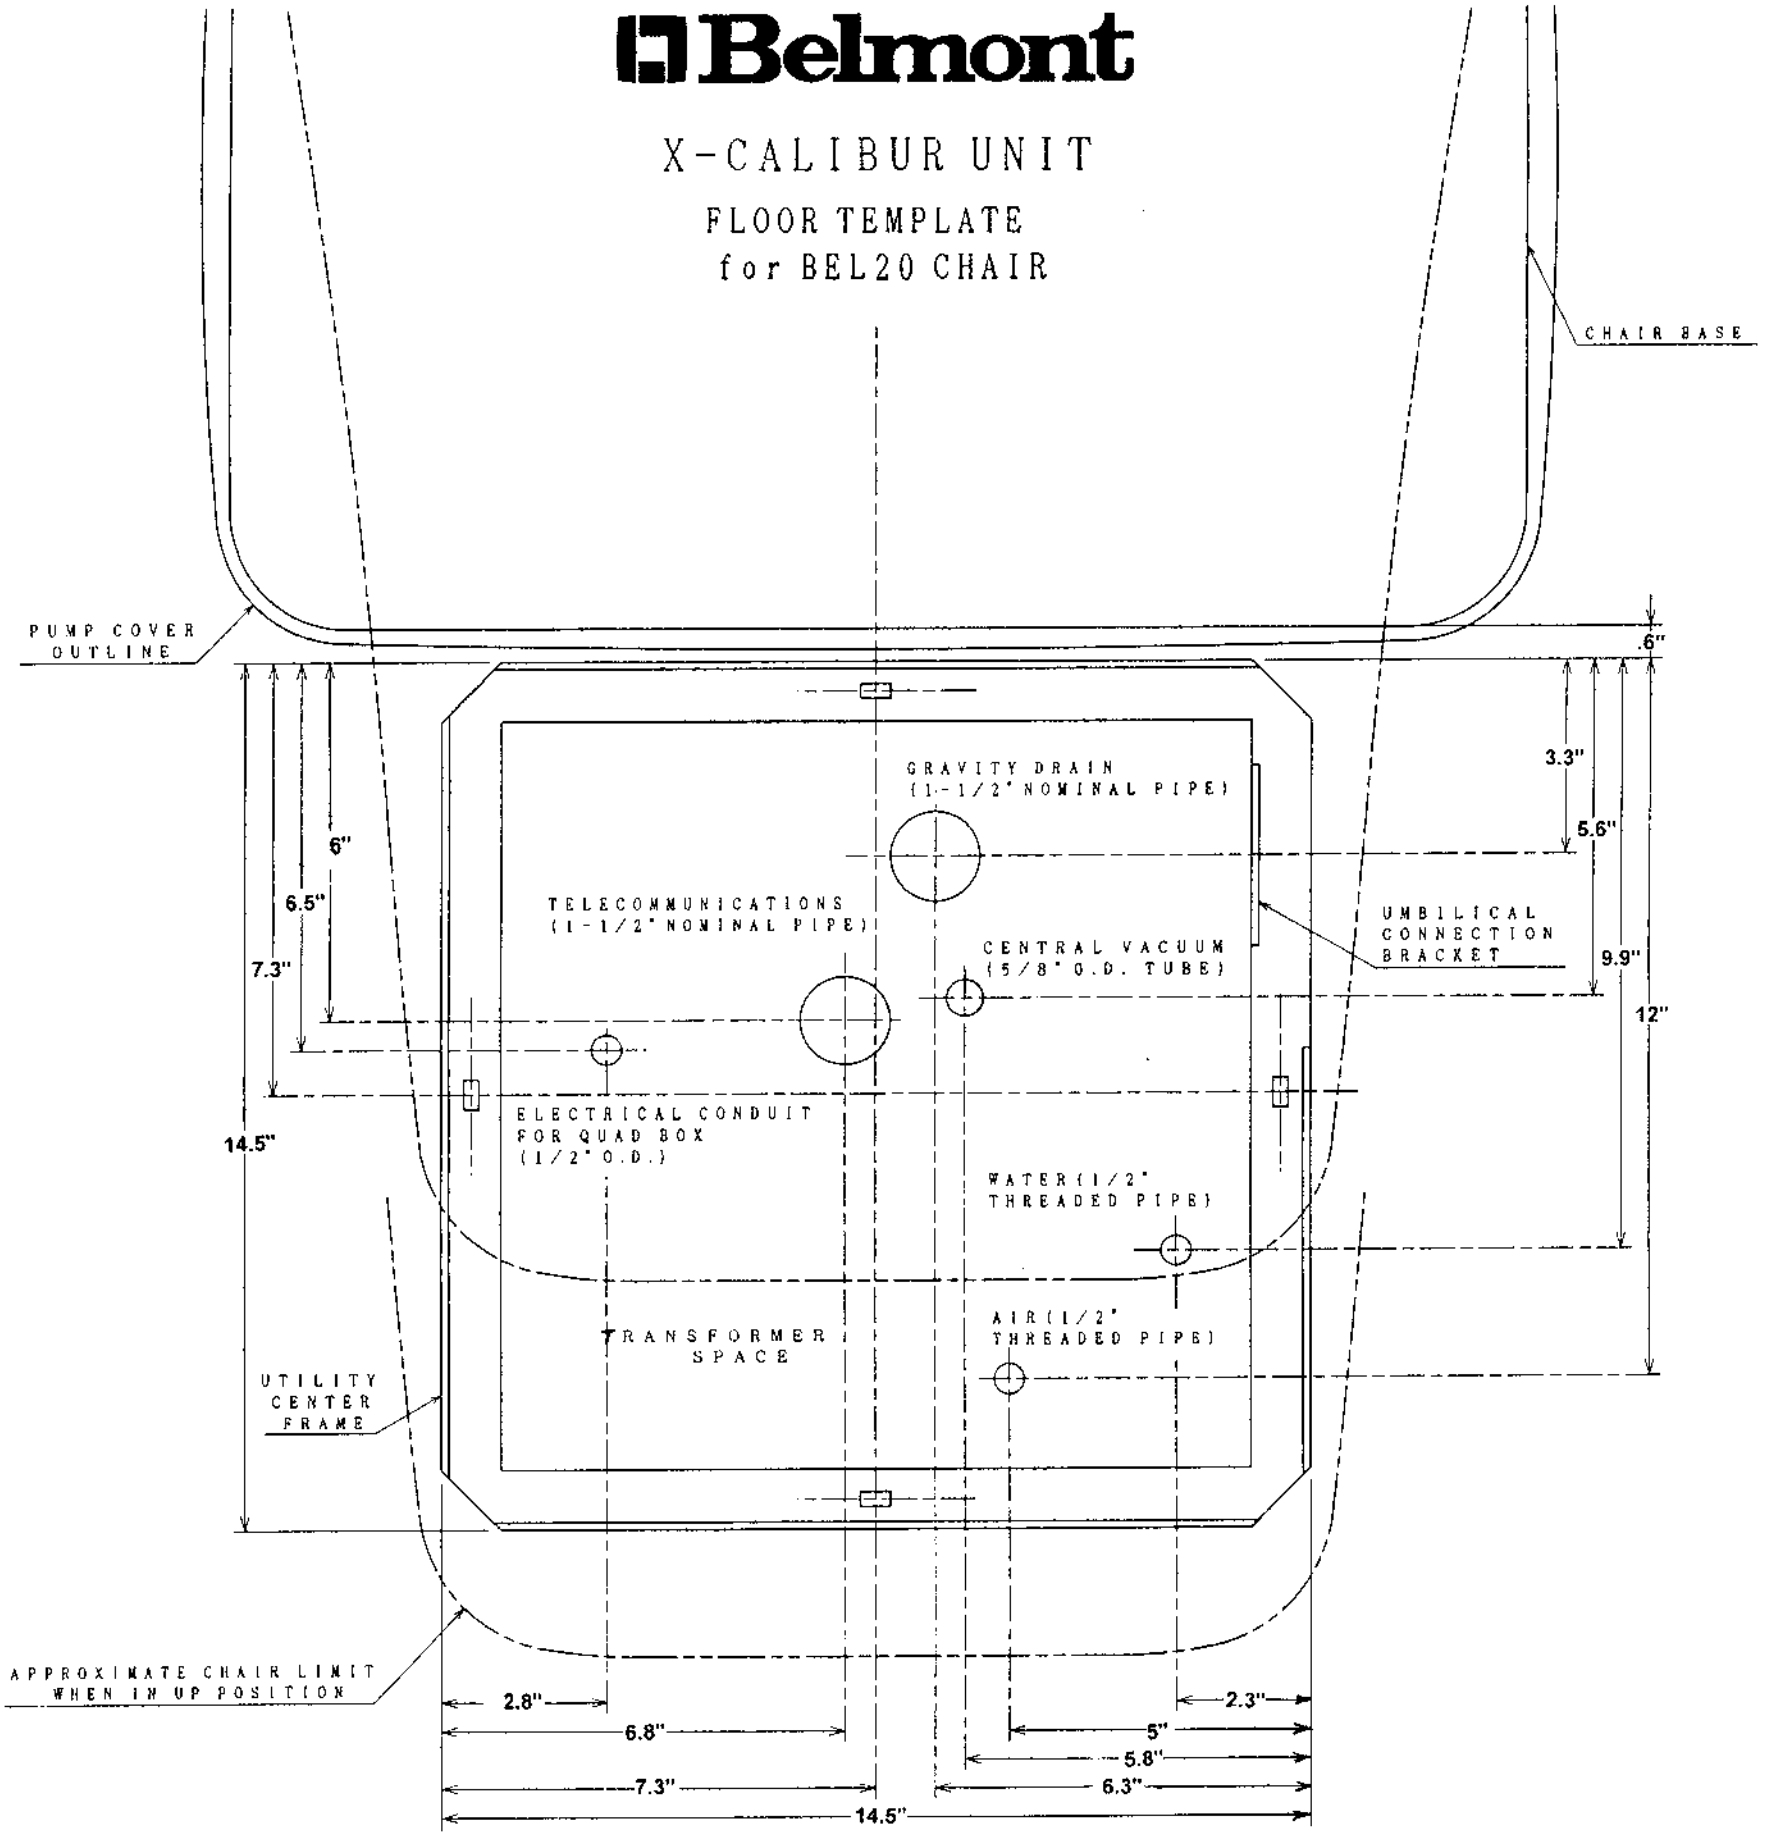

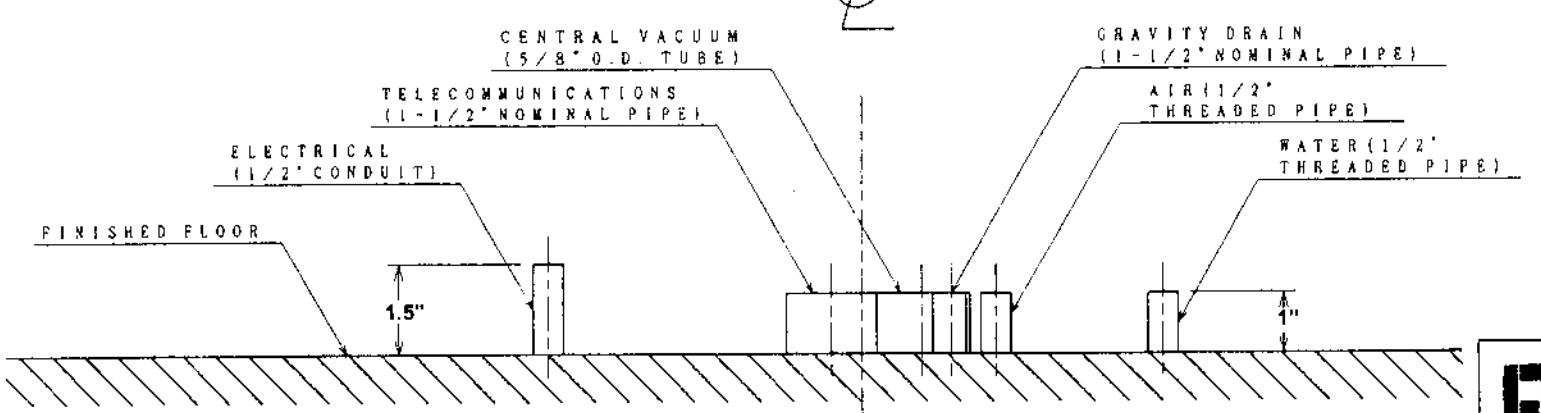

NOTES:
①LOCAL REGULATIONS PROVIDE THAT LICENSED PLUMBERS+ELECTRICIANS SHALL INSTALL UTILITIES
②MAKE SURE ALL PLUMBING CONFORMS TO PREVAILING LOCAL CODES.
③PLUMBING CENTRAL VACUUM TO THE UTILITY CENTER SHOULD BE SPECIFIED BY THE CENTRAL VACUUM SUPPLIER AND TERMINATED IN UTILITY CENTER WITH5/8" O.D. TUBE PERPENDICULAR TO THE FLOOR, SIMILAR TO THE DRAIN CONNECTION.
④GRAVITY DRAIN HAS 1-1/2" NOMINAL PIPE PROTRUDING 1" FROM FINISHED FLOOR.
NOTE:CONTRACTOR TO SUPPLY AND PLACE TRAP IN LINE TO CONFORM WITH LOCAL CODES.
⑤ELECTRICAL CONTRACTOR TO SUPPLY QUAD ELECTRICAL OUTLET BOX.

Belmont

X-CALIBUR UNIT

FLOOR TEMPLATE
for BEL20 CHAIR